



## City Research Online

### City, University of London Institutional Repository

---

**Citation:** Phillips, J. P., George, K., Kyriacou, P. A. & Langford, R. M. (2009). Investigation of Photoplethysmographic Changes using a Static Compression Model of Spinal Cord Injury. Paper presented at the EMBC 2009. Annual International Conference of the IEEE, 3-6 Sept. 2009, Minneapolis, MN. doi: 10.1109/IEMBS.2009.5334166

This is the accepted version of the paper.

This version of the publication may differ from the final published version.

---

**Permanent repository link:** <https://openaccess.city.ac.uk/id/eprint/13438/>

**Link to published version:** <https://doi.org/10.1109/IEMBS.2009.5334166>

**Copyright:** City Research Online aims to make research outputs of City, University of London available to a wider audience. Copyright and Moral Rights remain with the author(s) and/or copyright holders. URLs from City Research Online may be freely distributed and linked to.

**Reuse:** Copies of full items can be used for personal research or study, educational, or not-for-profit purposes without prior permission or charge. Provided that the authors, title and full bibliographic details are credited, a hyperlink and/or URL is given for the original metadata page and the content is not changed in any way.

---

City Research Online:

<http://openaccess.city.ac.uk/>

[publications@city.ac.uk](mailto:publications@city.ac.uk)

---

# Investigation of Photoplethysmographic Changes using a Static Compression Model of Spinal Cord Injury

Justin P. Phillips, *Member, IEEE*, Kuriakose J. George, Panayiotis A. Kyriacou, *Senior Member, IEEE*, and Richard M. Langford.

**Abstract**— Little is known about cell death in spinal cord tissue following compression injury, despite compression being a key component of spinal injuries. Currently models are used to mimic compression injury in animals and the effects of the compression evaluated by observing the extent and duration of recovery of normal motor function in the days and weeks following the injury. A fiber-optic photoplethysmography system was used to investigate whether pulsation of the small arteries in the spinal cord occurred before, during and after compressive loads were applied to the tissue. It was found that the signal amplitudes were reduced and this reduction persisted for at least five minutes after the compression ceased. It is hoped that results from this preliminary study may improve knowledge of the mechanism of spinal cord injury.

## I. INTRODUCTION

The mechanism through which spinal cord injury (SCI) can occur is complex. Compression injury is a key component of natural spinal injuries and is caused by displacement of the vertebral bones or discs. The compression can give rise to hemorrhage, edema and ischemia which can cause further injury after the initial impact [1]. Such secondary injury can cause serious permanent loss of function, however appropriate and rapid hospital treatment can potentially minimize this damage component.

Several models have been developed to investigate various SCI mechanisms in adult rats. Such models mimic the effects of primary injury, mostly due to laceration and contusion [2]. Other models, such as that used in the current study, provide quantitative information on the effect of compression on neuronal damage and subsequent recovery. A section of spinal cord is usually exposed in anesthetized animals. The recovery of the animals is monitored in the days following several minutes' controlled compression of the exposed section of the cord. The exact mechanism through which neuronal damage occurs during and after the compression is uncertain, and the extent to which ischemia contributes to the injury is not known.

J. P. Phillips and P.A. Kyriacou are with the School of Engineering and Mathematical Sciences, City University, London, EC1V 0HB, UK (e-mail: justin.phillips.1@city.ac.uk).

K. J. George was with the Neuroscience Centre, Queen Mary, University of London, E1 0NS, UK (email:kjoshigeorge@yahoo.co.uk).

R. M. Langford is with the Anaesthetic Laboratory, St Bartholomew's Hospital, London, EC1A 7BE, UK (e-mail: r.m.langford@btconnect.com).

A study was undertaken to measure photoplethysmographic (PPG) signals from the spinal cords of anesthetized rats before, during and after compression. These animals were used for ongoing compression model studies and the apparatus was modified to incorporate a fiber-optic probe for measuring the PPG waveforms. This pilot study was performed to investigate whether PPG signals are useful for assessing whether blood supply is disrupted during compression of the spinal cord and in the period immediately after compression.

## II. MATERIALS AND METHODS

### A. Measurement system

The measurement system for this study [3], [4] was developed and evaluated in our laboratory, based around a fiber-optic reflectance PPG probe. The probe consisted of two silica optical fibers (a transmitting fiber and a receiving fiber) each with a core diameter of 400  $\mu\text{m}$ , an outer cladding diameter of 730  $\mu\text{m}$  and a numerical aperture (NA) of 0.39 (Ocean Optics Inc., Dunedin, FL, USA). One of the fibers was used to transmit light from an LED with a peak emission wavelength 850 nm to the tissue and the other to return a fraction of the backscattered light to a photodiode. The centres of the two fibers were laterally separated by a distance of 1.0 mm. The distal end of each fiber was cut and polished flat and the proximal end terminated with a male SMA connector. The fibers were coated in a protective PVC jacket, which was stripped away over a length of several centimetres from the distal end.

A signal processing system was interfaced to a 16-bit data acquisition card (National Instruments Inc., Austin, TX, USA) installed into a notebook computer. A LabVIEW (National Instruments Inc., Austin, TX, USA) was implemented to display and record the acquired PPG signals.

### B. Static compression system

Apparatus developed for a well-established static compression system [5], [6], [7], [8] was adapted for this study. The apparatus consists of a stereotactic frame which holds the animal so that the spinal cord is maintained in a horizontal position. A metal bar measuring ( $h \times l \times w$ ) 1.5 mm  $\times$  5 mm  $\times$  3 mm attached to a platform on which a 50 g weight is placed is used for the compression as shown in Figure 1. The metal tube connecting the bar to the platform is supported within the stereotactic frame in such a way that

it is free to move in the vertical direction only.

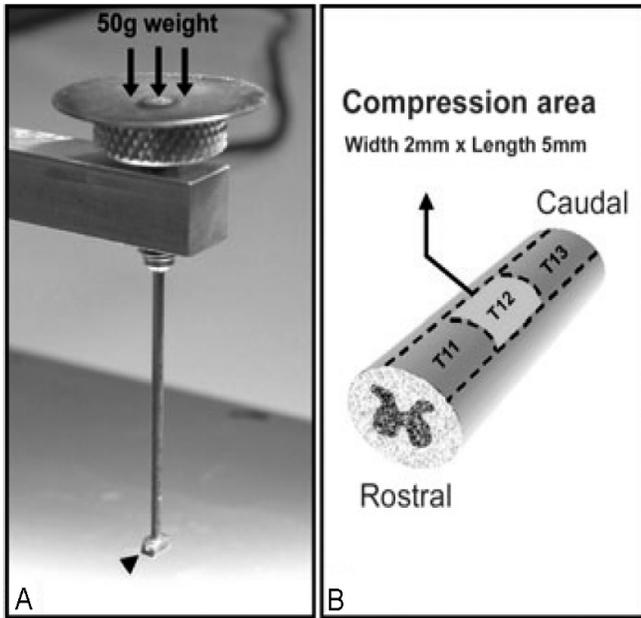


Fig. 1. Apparatus for rat spinal cord compression. (A) compression bar and weight. (B) section of spinal cord showing compression area (light gray). Adapted from Huang et al. [3].

The fiber optic PPG probe was passed along the metal tube attached to the compression bar. The fiber ends were inserted into the bar so they were flush with the lower surface of the bar as shown in Figure 2. The lower surface of the bar is curved to fit the contour of the rat spinal cord thus avoiding any localized compression of the tissue. The proximal ends of the fibers were connected to the measurement system.

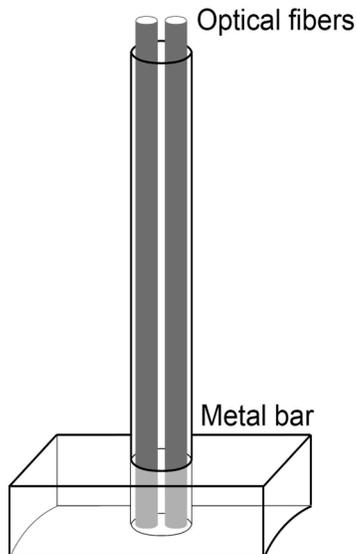


Fig. 2. Compression bar with optical fibers inserted.

### C. Measurements

All experimental protocols of this study were approved by the animal care committee of Queen Mary University of London, UK in accordance with the UK Animals (Scientific Procedures) Act 1986 and international guidelines on the ethical use of animals.

The spinal cords of 6 female Sprague–Dawley rats weighing approximately 250 g were used for this study. The rats were deeply anesthetized in a fume box with a mixture of 5% Halothane (Meril, Essex, UK) in addition to a mixture of oxygen and nitrous oxide (1 : 1 ratio) at a flow rate of 750–1000 mL/min. Subsequent anesthesia throughout the procedure was maintained using 1.5–2% halothane with oxygen and nitrous oxide at unchanged ratio delivered through a nose-piece. The skin and muscle overlying the spinal column were incised and a laminectomy was then performed at T12, leaving the dura undisturbed.

The T11 and T13 spinal processes were clamped in a spinal compression frame, and the bar was placed in light contact with the spinal cord by suspending the base of the compression platform (area  $2 \times 5$  mm, Fig. 1B) onto the exposed T12 cord dura under microscopic control. Measurements were recorded from the PPG system for 5 minutes. A weight of 50 g was then applied statically to the platform for exactly 5 minutes, during which time PPG signal recording continued. The weight was then removed and PPG signals recorded for a further 5 minutes. The platform was then removed, the muscle layers were sutured and the skin layers closed with wound clips.

The amplitudes of the acquired PPG signals were measured using a fast Fourier transform algorithm. The PPG amplitudes from each subject were averaged over three five-minute epochs named: ‘Baseline’, ‘Compression’ and ‘Recovery’. The PPG amplitudes from the ‘Compression’ and ‘Recovery’ epochs were compared with the amplitude recorded during ‘Baseline’.

### III. RESULTS

Good quality PPG signals were achieved consistently from all six animals. Figure 3 shows a five-second sample of a PPG signal from the spinal cord dura of one subject.

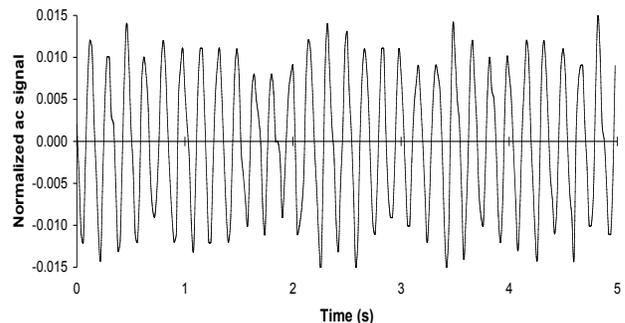


Fig. 3. Five-second sample of the PPG signal from the rat spinal cord dura.

An example of the waveform obtained for the entire 15-

minute measurement period is shown in Figure 4. It can be seen that in this example, the amplitude of the PPG signal decreased dramatically on compression. The PPG signal was attenuated for the duration of the compression. When the compression was relieved, the PPG amplitude increased to roughly two-thirds of its baseline value and then gradually increased. After five minutes the PPG amplitude was approximately equal to the baseline value.

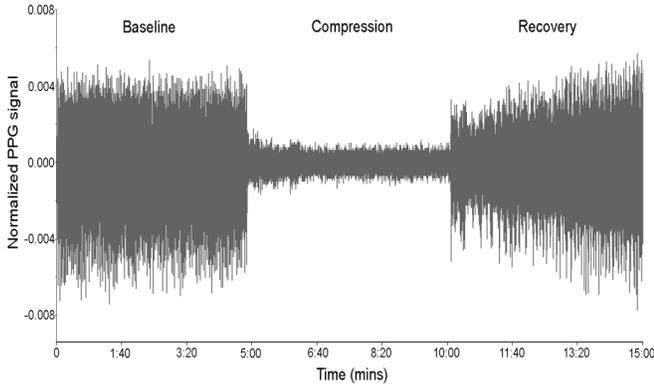


Fig. 4. 15-minute recording of PPG from the spinal cord before, during and after compression.

Figure 5 shows a graph of the PPG amplitude averaged over all three epochs for all six animals. It can be seen that all six animals showed a reduction in average PPG amplitude from baseline following compression of the cord. Four out of the six animals showed a subsequent increase in PPG amplitude when the compression weight was removed.

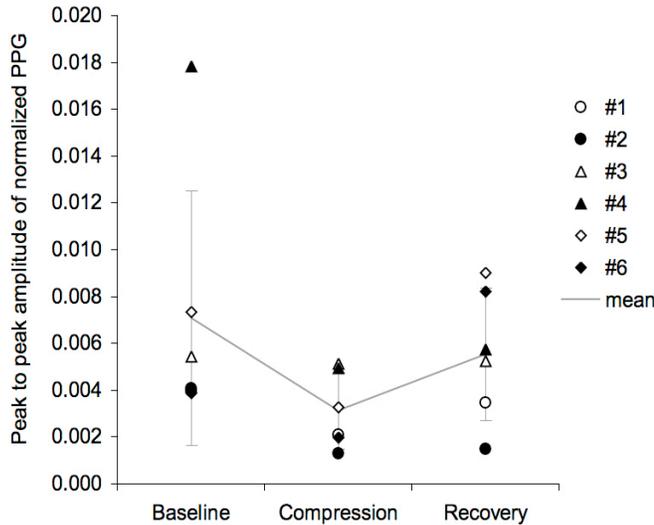


Fig. 5. Graph of the PPG amplitude averaged over 'Baseline', 'Compression' and 'Recovery' epochs for all six animals.

The mean reduction in PPG amplitude on compression was  $-55.9\%$  of the baseline value for all subjects. After removal of the compression weight, the mean PPG amplitude returned to  $-21.9\%$  of the baseline value. Although recovery

of the mean PPG amplitude was seen after removal of the compression weight for the population as a whole, a paired Student's t-test demonstrated that the increase in amplitude (from the 'Compression' state to the 'Recovery' state) was not significant ( $P=0.085$ ).

All six rats recovered to normal motor function within 0-3 days, suggesting that the compression of the spinal cord was not sufficient to cause permanent injury.

#### IV. DISCUSSION

It was found that good quality infrared PPG signals could be obtained from the spinal cord dura using a fiber-optic probe during static compression model measurements in rats. Compression of the spinal cord resulted in reduced pulsation indicated by attenuation of the PPG signal amplitude. This suggests that ischemia may occur during compressive injury. The reduction in PPG amplitude persisted even after removal of the compressive load, suggesting a further potential mechanism for secondary injury. Although the amplitude of the PPG signal gives an indication of the degree of arterial pulsation in the tissue vasculature, it should be noted that no information regarding the blood flow rate may be inferred from the PPG signal [9].

The next stage in the development of this project will be a trial using a larger number of subjects exposed to different compression loads. The spinal cord, like the brain, is one of the most vascular tissues in the human body and also among the most vulnerable to small changes in blood oxygenation. A comparison of PPG amplitude attenuation and recovery of motor function may hopefully shed light on the likely extent of ischemia in compressive spinal cord injury. Addition of a second wavelength to the measurement system should allow measurement of arterial oxygen saturation of blood within the tissue, which will indicate whether hypoxia is present during and after compression.

#### REFERENCES

- [1] A. P. Amar and M. L. Levy, "Pathogenesis and pharmacological strategies for mitigating secondary damage in acute spinal cord injury," *Neurosurgery*, vol. 44, pp. 1027-39; discussion 1039-40, May 1999
- [2] M. J. Crowe, J. C. Bresnahan, S. L. Shuman, J. N. Masters, and M. S. Beattie, "Apoptosis and delayed degeneration after spinal cord injury in rats and monkeys.[erratum appears in Nat Med 1997 Feb;3(2):240]," *Nature Medicine*, vol. 3, pp. 73-6, Jan 1997
- [3] J. P. Phillips, P. A. Kyriacou, K. J. George, J. V. Priestley, and R. M. Langford, "An optical fiber photoplethysmographic system for central nervous system tissue," *Conference Proceedings: ... Annual International Conference of the IEEE Engineering in Medicine & Biology Society*, vol. 1, pp. 803-6, 2006
- [4] J. P. Phillips, R. M. Langford, P. A. Kyriacou, and D. P. Jones, "Preliminary evaluation of a new fibre-optic cerebral oximetry system," *Physiological Measurement*, vol. 29, pp. 1383-1396, December 2008
- [5] B. Nystrom, J. E. Berglund, and E. Bergquist, "Methodological analysis of an experimental spinal cord compression model in the rat," *Acta Neurologica Scandinavica*, vol. 78, pp. 460-6, Dec 1988
- [6] G. L. Li, G. Brodin, M. Farooque, K. Funayama, A. Holtz, W. L. Wang, and Y. Olsson, "Apoptosis and expression of Bcl-2 after compression trauma to rat spinal cord," *Journal of Neuropathology & Experimental Neurology*, vol. 55, pp. 280-9, Mar 1996

- [7] W. L. Huang, D. Robson, M. C. Liu, V. R. King, S. Averill, P. J. Shortland, and J. V. Priestley, "Spinal cord compression and dorsal root injury cause up-regulation of activating transcription factor-3 in large-diameter dorsal root ganglion neurons," *European Journal of Neuroscience*, vol. 23, pp. 273-8, Jan 2006
- [8] W. L. Huang, K. J. George, V. Ibba, M. C. Liu, S. Averill, M. Quartu, P. J. Hamlyn, and J. V. Priestley, "The characteristics of neuronal injury in a static compression model of spinal cord injury in adult rats," *European Journal of Neuroscience*, vol. 25, pp. 362-72, Jan 2007
- [9] N. E. Almond, D. P. Jones, and E. D. Cooke, "Noninvasive measurement of the human peripheral circulation: relationship between laser Doppler flowmeter and photoplethysmograph signals from the finger," *Angiology*, vol. 39, pp. 819-29, Sep 1988