



## City Research Online

### City, University of London Institutional Repository

---

**Citation:** Charlton, P. H., Pilt, K. & Kyriacou, P. A. (2022). Establishing best practices in photoplethysmography signal acquisition and processing. *Physiological Measurement*, 43(5), 050301. doi: 10.1088/1361-6579/ac6cc4

This is the draft version of the paper.

This version of the publication may differ from the final published version.

---

**Permanent repository link:** <https://openaccess.city.ac.uk/id/eprint/28156/>

**Link to published version:** <https://doi.org/10.1088/1361-6579/ac6cc4>

**Copyright:** City Research Online aims to make research outputs of City, University of London available to a wider audience. Copyright and Moral Rights remain with the author(s) and/or copyright holders. URLs from City Research Online may be freely distributed and linked to.

**Reuse:** Copies of full items can be used for personal research or study, educational, or not-for-profit purposes without prior permission or charge. Provided that the authors, title and full bibliographic details are credited, a hyperlink and/or URL is given for the original metadata page and the content is not changed in any way.

---

---

---

City Research Online:

<http://openaccess.city.ac.uk/>

[publications@city.ac.uk](mailto:publications@city.ac.uk)

---



## EDITORIAL

## Establishing best practices in photoplethysmography signal acquisition and processing

## OPEN ACCESS

PUBLISHED  
25 May 2022

Original content from this work may be used under the terms of the [Creative Commons Attribution 4.0 licence](#).

Any further distribution of this work must maintain attribution to the author(s) and the title of the work, journal citation and DOI.

Peter H Charlton<sup>1,2,\*</sup> , Kristjan Pilt<sup>3</sup>  and Panicos A Kyriacou<sup>2</sup> <sup>1</sup> Department of Public Health and Primary Care, University of Cambridge, United Kingdom<sup>2</sup> Research Centre for Biomedical Engineering, City, University of London, United Kingdom<sup>3</sup> Department of Health Technologies, Tallinn University of Technology, Ehitajate tee 5, 19086 Tallinn, Estonia

\* Author to whom any correspondence should be addressed.


E-mail: [pc657@medschl.cam.ac.uk](mailto:pc657@medschl.cam.ac.uk)**Abstract**

Photoplethysmography is now widely utilised by clinical devices such as pulse oximeters, and wearable devices such as smartwatches. It holds great promise for health monitoring in daily life. This editorial considers whether it would be possible and beneficial to establish best practices for photoplethysmography signal acquisition and processing. It reports progress made towards this, balanced with the challenges of working with a diverse range of photoplethysmography device designs and intended applications, each of which could benefit from different approaches to signal acquisition and processing. It concludes that there are several potential benefits to establishing best practices. However, it is not yet clear whether it is possible to establish best practices which hold across the range of photoplethysmography device designs and applications.

This Editorial considers whether it would be possible and beneficial to establish best practices for acquiring and processing photoplethysmography signals.

Photoplethysmography is an optical technique which provides non-invasive measurements of the arterial pulse wave, which is related to the blood volume change in the observed microvascular tissue. The photoplethysmogram (PPG) signal is already widely utilised by clinical devices such as pulse oximeters (Alian and Shelley), and wearable devices such as smartwatches (Charlton and Marozas). Photoplethysmography holds great promise for health monitoring in daily life. Indeed, several potential applications of photoplethysmography were presented in 2021 alone in *Physiological Measurement*, including: blood pressure monitoring (Esmalpoor *et al* 2021, Xing *et al* 2021); detecting peripheral arterial disease (Allen *et al* 2021); sleep staging (Li *et al* 2021); screening for sleep apnea and cardiovascular disease (Behar *et al* 2020, Ouyang *et al* 2021); and detecting driver sleepiness (Hultman *et al* 2021).

Despite the widespread use of photoplethysmography, best practices have not yet been established for acquiring and processing photoplethysmography signals. This may in part be due to the diversity of photoplethysmography device designs, ranging from smartwatches to earbuds, and applications, ranging from oxygen saturation measurement in clinical practice to heart rate monitoring during exercise (Charlton *et al* 2022). Potentially, the best approach to signal acquisition and signal processing could differ between each device design and application. Nonetheless, there could be benefits to establishing best practices, such as establishing hardware configurations that consistently provide high quality signals, and establishing signal processing algorithms that can accurately derive parameters from a variety of PPG signals. This is illustrated by the findings of Liu *et al* in their recent article in *Physiological Measurement*. They found that the use of different PPG signal filtering settings can result in different measurements being obtained from PPG pulse wave analysis. Based on this, they highlighted the potential benefits of the ‘standardisation’ of PPG filtering (Liu *et al* 2021). In this case, establishing best practices for filtering PPG signals would have the benefit of allowing pulse wave indices to be compared between studies and between devices. However, this may not be straightforward as different filtering settings may be required for different applications, such as heart rate monitoring (which uses the fundamental frequency of the PPG,  $\approx 0.5\text{--}3\text{Hz}$ ) and blood pressure assessment (which uses higher frequency content).

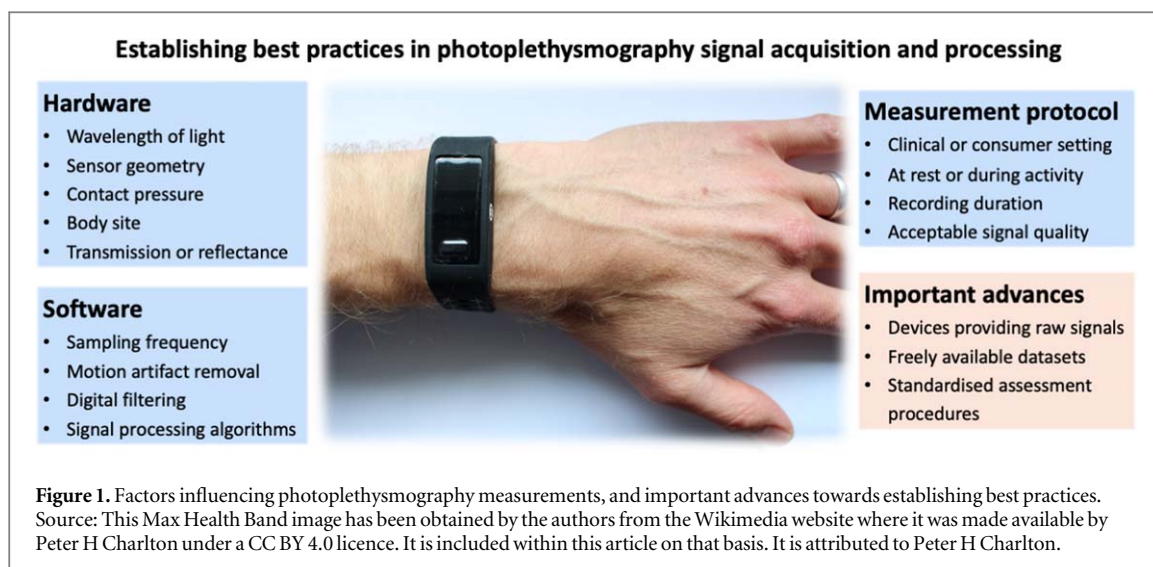

Potential areas in which best practices could be established include factors relating to device design (hardware and software) and measurement protocols (recording setting and duration). These are summarised in figure 1, and now described.

Several factors in the hardware design influence the PPG signal (Charlton and Marozas, Lemay *et al*), and are therefore potential areas in which best practices could be established. Firstly, the wavelength of emitted light determines the depth of light penetration, and consequently the level of the vasculature contributing to the PPG signal (Liu *et al* 2019), which influences signal quality (Fallow *et al* 2013). Current best practice is to use longer wavelengths (e.g. infrared) for transmission photoplethysmography as these penetrate deeper (Anderson and Parrish 1981), and shorter wavelengths (e.g. green) for reflectance photoplethysmography as these produce higher signal quality for heart rate measurement (Matsumura *et al* 2020). However, this practice may need to be revisited as the use of green light has been found to result in less accurate heart rate monitoring in subjects with darker skin tones (Fine *et al*). Secondly, in reflectance photoplethysmography the signal quality is influenced by the geometry of the light emitter, light detector, and sensor casing. Current best practice is to design the surrounding casing to eliminate ambient light as far as possible (Abay and Kyriacou). In the future this may be extended to using geometries in which the LED surrounds the photo detector, as these have been found to give higher signal quality (Khan *et al* 2019). Thirdly, the contact pressure applied by the device to the skin impacts the shape of the PPG pulse wave (Chandrasekhar *et al* 2020) and consequently its second derivative (Grabovskis *et al* 2013). Best practice in the area of contact pressure has not yet been established: higher pressures may reduce probe-tissue movement artifact, and have been found to increase the accuracy of PPG-based heart rate monitoring (Scardulla *et al* 2020). However, it is not clear whether such pressures would be suitable for long-term monitoring. Ideally, the contact pressure should remain constant when analysing pulse wave shape, such as when tracking changes nocturnal changes in blood pressure (Radha *et al* 2019). Fourthly, the body site chosen for PPG measurement influences pulse wave shape (Hartmann *et al* 2019), and the utility of the acquired signal (Charlton and Marozas). Best practice has not yet been established in this area: in clinical devices the finger is often used (Alty *et al* 2007), whereas in consumer devices the wrist is often used due to user preference (Prinable *et al* 2017). In summary, the challenge of establishing best practices is not trivial, as several factors can influence the PPG signal, and it is likely that different device configurations would be best suited to different applications.

The software used in PPG devices influences the PPG signal and the parameters derived from it, and therefore presents potential areas in which to establishing best practices. Firstly, there is a compromise between increasing the sampling frequency to capture details of the shape of PPG pulse waves, and reducing it to reduce power consumption (Lee *et al* 2018). Best practices differ between applications, with minimum acceptable sampling frequencies of 10, 16, and 25 Hz reported for heart rate, respiratory rate, and pulse rate variability measurements respectively (Wolling and Van Laerhoven, Charlton *et al* 2017, Choi and Shin 2017). Secondly, different approaches can be used to remove motion artifact, ranging from eliminating periods of motion (Guo *et al* 2021), to denoising the PPG (Zhang *et al* 2015), to cancelling motion artifact using a reference accelerometer or gyroscope signal (Marozas and Charlton 2021). Here, best practices also differ between applications: in hospital monitoring it has been proposed that periods of motion should be eliminated from analyses (Orphanidou *et al* 2015), whereas in exercise monitoring the alternative approaches of denoising the PPG or cancelling motion artifact are used (Zhang *et al* 2015). Whilst it may be challenging to develop a universal strategy to PPG signal quality assessment, recent work has demonstrated that a single approach can perform well

across different heart rhythms and different PPG devices (Mohagheghian *et al*). Thirdly, the analog and digital filtering used to pre-process signals influences both the amplitudes and timings of PPG pulse wave features (Liang *et al* 2018, Liu *et al* 2021). For instance, an optimal low-pass filter cut-off of 6 Hz has been proposed to preserve the higher harmonic components of the PPG, and minimise variability in indices calculated from its second derivative (Pilt *et al* 2013). Fourthly, the choice of signal processing algorithm used to estimate a physiological parameter from the signal can greatly influence the accuracy and precision of the parameter (Charlton *et al* 2016). Best practices for deriving pulse wave features from finger PPG signals have been proposed (Elgendi 2014, Elgendi *et al* 2014). However, best practices have not yet been established for signals acquired at the wrist, which differ from finger signals (Rajala *et al* 2018). Similarly, it could be beneficial to optimise neural network architectures for PPG analyses, building on existing architectures (Li *et al* 2021). Further work is also required to identify the best pulse wave features for different tasks from amongst the wide range of features proposed in the literature (Charlton *et al* 2018, Lin *et al* 2020). For instance, recent studies have investigated the best features for blood pressure estimation (Xing *et al* 2021) and pulse rate variability analysis (Peralta *et al* 2019). The best algorithm design may also depend on a subject's characteristics, as shown by recent proposals of different blood pressure estimation algorithms for subjects of different ages (Xing *et al* 2020) and subjects of different blood pressure categories (Khalid *et al* 2020). In summary, it may be difficult to establish best practices for the software used in PPG devices, as the best approach may vary according to the sensor configuration, application, and subjects being monitored.

A further area in which best practices could be established is the protocols used to obtain PPG measurements, where best practices could be used to obtain repeatable and reproducible measurements. Measurement protocols can be tightly controlled in clinical settings, where consideration can be given to room temperature, subject position, and the duration of rest prior to measurement (Allen and Hedley 2019). However, protocols cannot be so tightly controlled when obtaining measurements from consumer devices in daily life. Nevertheless, measurements can be obtained in a repeatable manner during periods of rest, such as resting and night-time resting heart rates (Mishra *et al* 2020, Radin *et al* 2020). Future work may consider the required recording durations and acceptable levels of signal quality to estimate different physiological parameters from the PPG (Huthart *et al* 2020). Whilst it is possible to obtain some parameters during exercise (e.g. heart rate) (Zhang *et al* 2015), it may only be possible to obtain other parameters accurately whilst at rest (e.g. those derived from the second derivative of the PPG, such as the aging index) (Takazawa *et al* 1998).

It is clear that there are several potential areas in which best practices could be established for the acquisition and processing of PPG signals. However, it is not yet clear whether it would be possible and beneficial to establish best practices. On the one hand: it may not be possible to establish best practices as they may vary greatly between device designs and applications; it may not be possible to use them widely if they are patented; and, they may not be beneficial if they don't substantially improve device performance. On the other hand, establishing best practices could: reduce the time taken to design and manufacture devices; ensure PPG-based measurements are as accurate and reproducible as possible; and, help advance the field as researchers and developers could build on existing best practices when making novel developments.

Several advances could aid research into determining whether it would be possible and beneficial to establish best practices for PPG signal acquisition and processing. Firstly, wearable devices which provide the raw PPG signal are invaluable for such research, as demonstrated through the use of the Empatica E4 wristband in many research studies (McCarthy *et al*). Whilst several research devices can provide the raw PPG signal (Charlton *et al* 2022), large-scale studies could be conducted more easily in daily life if consumer devices were similarly able to provide raw PPG signals. Secondly, freely available datasets allow researchers to benchmark their own PPG signal processing algorithms against others on a common dataset. Several such datasets are available (Charlton *et al* 2022), including: the WeSAD and PPG-DaLiA datasets, acquired using an Empatica E4 device in healthy subjects (Schmidt *et al*, Reiss *et al* 2019); and the VitalDB and the MIMIC Waveform databases, acquired from critically-ill patients (Johnson *et al* 2016, Lee and Jung 2018). However, there are limitations to current datasets: they are often collected from either healthy volunteers or a particular patient population, rather than a broad cross-section of society; they often contain PPG signals acquired by only one device, rather than signals acquired using different hardware configurations; and they are often recorded in either laboratory or clinical settings, but few are recorded in daily life. Thirdly, there is a need for widely accepted validation protocols with which to assess the performance of PPG-based devices. Such protocols already exist for devices measuring blood pressure and heart rate (Stergiou *et al* 2018, Mühlen *et al* 2021). However, different standards may be required for different applications, such as varying the accuracy and data availability thresholds according to the intended use case and measurement scenario (Consumer Technology Association 2018, Mukkamala *et al* 2021).

To conclude, there are several potential benefits to establishing best practices for acquiring and processing PPG signals. However, it is not yet clear whether it is possible to establish best practices which hold across the range of PPG device designs and applications. Therefore, much further work is required to investigate whether it

would be possible and beneficial to establish best practices, and to understand how they may differ between device designs and intended applications.

## Acknowledgments

This paper is based upon work from COST ACTION CA18216 ‘Network for Research in Vascular Ageing’, supported by COST (European Cooperation in Science and Technology): [www.cost.eu](http://www.cost.eu). The work was supported by British Heart Foundation (BHF) Grant FS/20/20/34626, and by the Estonian Ministry of Education and Research under personal post-doctoral research funding PUTJD815. Certain images in this publication have been obtained by the authors from the Wikimedia website, where they were made available under a Creative Commons licence. Please see individual figure captions in this publication for details. To the extent that the law allows, IOP Publishing and Institute of Physics and Engineering in Medicine disclaim any liability that any person may suffer as a result of accessing, using or forwarding the image(s). Any reuse rights should be checked and permission should be sought if necessary from Wikimedia and/or the copyright owner (as appropriate) before using or forwarding the image(s).

## ORCID iDs

Peter H Charlton  <https://orcid.org/0000-0003-3836-8655>

Kristjan Pilt  <https://orcid.org/0000-0003-2422-0430>

Panicos A Kyriacou  <https://orcid.org/0000-0002-2868-485X>

## References

- Abay T Y and Kyriacou P A 2022 Photoplethysmography in oxygenation and blood volume measurements *Photoplethysmography: Technology, Signal Analysis, and Applications* ed P A Kyriacou and J Allen (Amsterdam: Elsevier) Ch. 5 pp 147–88
- Alian A A and Shelley K H 2022 PPG in clinical monitoring *Photoplethysmography: Technology, Signal Analysis and Applications* ed P A Kyriacou and J Allen (Amsterdam: Elsevier) Ch.10 pp 341–59
- Allen J and Hedley S 2019 Simple photoplethysmography pulse encoding technique for communicating the detection of peripheral arterial disease - a proof of concept study *Physiol. Meas.* **40** 08NT01
- Allen J, Liu H, Iqbal S, Zheng D and Stansby G 2021 Deep learning-based photoplethysmography classification for peripheral arterial disease detection: a proof-of-concept study *Physiol. Meas.* **42** 054002
- Alty S R, Angarita-Jaimes N, Millasseau S C and Chowienczyk P J 2007 Predicting arterial stiffness from the digital volume pulse waveform *IEEE Trans. Biomed. Eng.* **54** 2268–75
- Anderson R R and Parrish J A 1981 The optics of human skin *J. Invest Dermatol* **77** 13–19
- Behar J A et al 2020 Remote health diagnosis and monitoring in the time of COVID-19 *Physiol. Meas.* **41** 10TR01
- Chandrasekhar A, Yavarimanesh M, Natarajan K, Hahn J-O and Mukkamala R 2020 PPG sensor contact pressure should be taken into account for cuff-less blood pressure measurement *IEEE Trans. Biomed. Eng.* **67** 3134–40
- Charlton P H, Bonnici T, Tarassenko L, Alastruey J, Clifton D A, Beale R and Watkinson P J 2017 Extraction of respiratory signals from the electrocardiogram and photoplethysmogram: technical and physiological determinants *Physiol. Meas.* **38** 669–90
- Charlton P H, Bonnici T, Tarassenko L, Clifton D A, Beale R and Watkinson P J 2016 An assessment of algorithms to estimate respiratory rate from the electrocardiogram and photoplethysmogram *Physiol. Meas.* **37** 610–26
- Charlton P H, Celka P, Farukh B, Chowienczyk P and Alastruey J 2018 Assessing mental stress from the photoplethysmogram: a numerical study *Physiol. Meas.* **39** 054001
- Charlton P H, Kyriacou P A, Mant J, Marozas V, Chowienczyk P and Alastruey J 2022 Wearable photoplethysmography for cardiovascular monitoring *Proc. IEEE* **110** 355–81
- Charlton P H and Marozas V 2022 Wearable photoplethysmography devices *Photoplethysmography: Technology, Signal Analysis and Applications* ed P A Kyriacou and J Allen (Amsterdam: Elsevier) Ch.12 pp 401–39
- Choi A and Shin H 2017 Photoplethysmography sampling frequency: pilot assessment of how low can we go to analyze pulse rate variability with reliability? *Physiol. Meas.* **38** 586–600
- Consumer Technology Association 2018 Physical Activity Monitoring for Heart Rate, ANSI/CTA 2065 [Online]. (<https://shop.cta.tech/collections/standards/products/physical-activity-monitoring-for-heart-rate>)
- Elgendi M 2014 Detection of c, d, and e waves in the acceleration photoplethysmogram *Comput. Methods Programs Biomed.* **117** 125–36
- Elgendi M, Norton I, Brearley M, Abbott D and Schuurmans D 2014 Detection of a and b waves in the acceleration photoplethysmogram *Biomed. Eng. Online* **13** 139
- Esmaelpoor J, Moradi M H and Kadkhodamohammadi A 2021 Cuffless blood pressure estimation methods: physiological model parameters versus machine-learned features *Physiol. Meas.* **42** 035006
- Fallow B A, Tarumi T and Tanaka H 2013 Influence of skin type and wavelength on light wave reflectance *J. Clin. Monit. Comput.* **27** 313–17
- Fine J, Branam KL, Rodriguez AJ, Boonya-Ananta T, Ajmal, Ramella-Roman JC, McShane MJ and Coté GL. 2021 Sources of inaccuracy in photoplethysmography for continuous cardiovascular monitoring *Biosensors* **11** 126
- Grabovskis A, Marcinkevics Z, Rubins U and Kvišis-Kipge E 2013 Effect of probe contact pressure on the photoplethysmographic assessment of conduit artery stiffness *J. Biomed. Opt.* **18** 027004
- Guo Z, Ding C, Hu X and Rudin C 2021 A supervised machine learning semantic segmentation approach for detecting artifacts in plethysmography signals from wearables *Physiol. Meas.* **42** 125003
- Hartmann V, Liu H, Chen F, Qiu Q, Hughes S and Zheng D 2019 Quantitative comparison of photoplethysmographic waveform characteristics: effect of measurement site *Front. Physiol.* **10** 198

- Hultman M, Johansson I, Lindqvist F and Ahlström C 2021 Driver sleepiness detection with deep neural networks using electrophysiological data *Physiol. Meas.* **42** 034001
- Huthart S, Elgendi M, Zheng D, Stansby G and Allen J 2020 Advancing PPG signal quality and know-how through knowledge translation—from experts to student and researcher *Front. Digit. Health* **2** 619692
- Johnson A E W, Pollard T J, Shen L, Lehman L H, Feng M, Ghassemi M, Moody B, Szolovits P, Anthony Celi L and Mark R G 2016 MIMIC-III, a freely accessible critical care database *Sci. Data* **3** 160035
- Khalid S G, Liu H, Zia T, Zhang J, Chen F and Zheng D 2020 Cuffless blood pressure estimation using single channel photoplethysmography: a two-step method *IEEE Access* **8** 58146–54
- Khan Y, Han D, Ting J, Ahmed M, Nagisetty R and Arias A C 2019 Organic multi-channel optoelectronic sensors for wearable health monitoring *IEEE Access* **7** 128114–24
- Lee H C and Jung C W 2018 Vital recorder- a free research tool for automatic recording of high-resolution time-synchronised physiological data from multiple anaesthesia devices *Sci. Rep.* **8** 1–8
- Lee J, Jang D H, Park S and Cho S H 2018 A low-power photoplethysmogram-based heart rate sensor using heartbeat locked loop *IEEE Trans. Biomed. Circuits Syst.* **12** 1220–9
- Lemay M, Bertschi M, Sola J, Renevey P, Genzoni E, Proença M, Ferrario D, Braun F, Parak J and Korhonen I. 2021 Applications of Optical Cardiovascular Monitoring *Wearable Sensors: Fundamentals, Implementation and Applications* (Amsterdam: Elsevier) Ch.18 pp 487–517
- Li Q, Li Q, Cakmak A S, Poian G D, Bliwise D L, Vaccarino V, Shah A J and Clifford G D 2021 Transfer learning from ECG to PPG for improved sleep staging from wrist-worn wearables *Physiol. Meas.* **42** 044004
- Liang Y, Elgendi M, Chen Z and Ward R 2018 An optimal filter for short photoplethysmogram signals *Sci. Data* **5** 1–12
- Lin W H, Li X, Li Y, Li G and Chen F 2020 Investigating the physiological mechanisms of the photoplethysmogram features for blood pressure estimation *Physiol. Meas.* **41** 044003
- Liu H, Allen J, Khalid S G, Chen F and Zheng D 2021 Filtering-induced time shifts in photoplethysmography pulse features measured at different body sites: the importance of filter definition and standardization *Physiol. Meas.* **42** 074001
- Liu J, Yan B P, Zhang Y, Ding X, Su P and Zhao N 2019 Multi-wavelength photoplethysmography enabling continuous blood pressure measurement with compact wearable electronics *IEEE Trans. Biomed. Eng.* **66** 1514–25
- Marozas V and Charlton P H 2021 Wearable Photoplethysmography Devices (Zenodo) (<https://doi.org/10.5281/zenodo.4601547>)
- Matsumura K, Toda S and Kato Y 2020 RGB and near-infrared light reflectance/transmittance photoplethysmography for measuring heart rate during motion *IEEE Access* **8** 80233–42
- McCarthy C, Pradhan N, Redpath C and Adler A 2016 Validation of the empatica E4 wristband 2016 *IEEE EMBS International Student Conference (ISC) (Ottawa, ON, Canada, 29-31 May 2016)* (IEEE) (<https://doi.org/10.1109/EMBSISC.2016.7508621>)
- Mishra T *et al* 2020 Pre-symptomatic detection of COVID-19 from smartwatch data *Nat. Biomed. Eng.* **4** 112208
- Mohagheghian F *et al* 2022 Optimized signal quality assessment for photoplethysmogram signals using feature selection *IEEE Transactions on Biomedical Engineering* **In Press**
- Mühlen J M *et al* 2021 Recommendations for determining the validity of consumer wearable heart rate devices: expert statement and checklist of the INTERLIVE network *Br. J. Sports Med.* **55** 767–79
- Mukkamala R, Yavarimanesh M, Natarajan K, Hahn J O, Kyriakoulis K G, Avolio A P and Stergiou G S 2021 Evaluation of the accuracy of cuffless blood pressure measurement devices: challenges and proposals *Hypertension* **78** 1161–67
- Orphanidou C, Bonnici T, Charlton P, Clifton D, Vallance D and Tarassenko L 2015 Signal-quality indices for the electrocardiogram and photoplethysmogram: derivation and applications to wireless monitoring *IEEE J. Biomed Health Inform.* **19** 83832–8
- Ouyang V, Ma B, Pignatelli N, Sengupta S, Sengupta P, Mungulmare K and Fletcher R R 2021 The use of multi-site photoplethysmography (PPG) as a screening tool for coronary arterial disease and atherosclerosis *Physiol. Meas.* **42** 064006
- Peralta E, Lazaro J, Bailon R, Marozas V and Gil E 2019 Optimal fiducial points for pulse rate variability analysis from forehead and finger photoplethysmographic signals *Physiol. Meas.* **40** 025007
- Pilt K, Ferenets R, Meigas K, Lindberg L-G, Temitski K and Viigimaa M 2013 New photoplethysmographic signal analysis algorithm for arterial stiffness estimation *Sci. World J.* **2013** 1–9
- Prinable J B, Foster J M, McEwan A L, Young P M, Tovey E and Thamrin C 2017 Motivations and key features for a wearable device for continuous monitoring of breathing: a web-based survey *JMIR Biomed. Eng.* **2** e1
- Radha M *et al* 2019 Estimating blood pressure trends and the nocturnal dip from photoplethysmography *Physiol. Meas.* **40** 025006
- Radin J M, Wineinger N E, Topol E J and Steinhubl S 2020 Harnessing wearable device data to improve state-level real-time surveillance of influenza-like illness in the USA: a population-based study *Lancet Digit. Health* **2** e85–93
- Rajala S, Lindholm H and Taipalus T 2018 Comparison of photoplethysmogram measured from wrist and finger and the effect of measurement location on pulse arrival time *Physiol. Meas.* **39** 075010
- Reiss A, Indlekofer I, Schmidt P and Van Laerhoven K 2019 Deep PPG: large-scale heart rate estimation with convolutional neural networks *Sensors* **19** 3079
- Scardulla F, D'acquisto L, Colombarini R, Hu S, Pasta S and Bellavia D 2020 A study on the effect of contact pressure during physical activity on photoplethysmographic heart rate measurements *Sensors* **20** 1–15
- Schmidt P, Reiss A, Duerichen R and Van Laerhoven K 2018 Introducing WeSAD, a multimodal dataset for wearable stress and affect detection *20th ACM International Conference on Multimodal Interaction (Boulder, CO, USA, 16 - 20 October 2018)* (New York, NY: Association for Computing Machinery) pp 400–8
- Stergiou G S *et al* 2018 A universal standard for the validation of blood pressure measuring devices: association for the Advancement of Medical Instrumentation/European Society of Hypertension/International Organization for Standardization (AAMI/ESH/ISO) Collaboration Statement *Hypertension* **71** 368–74
- Takazawa K, Tanaka N, Fujita M, Matsuoka O, Saiki T, Aikawa M, Tamura S and Ibukiyama C 1998 Assessment of vasoactive agents and vascular aging by the second derivative of photoplethysmogram waveform *Hypertension* **32** 365–70
- Wolling F and Van Laerhoven K 2018 Fewer samples for a longer life span *5th international Workshop on Sensor-based Activity Recognition and Interaction (Berlin, Germany, 20 - 21 September 2018)* (ACM) pp 1–10
- Xing X, Ma Z, Xu S, Zhang M, Zhao W, Song M and Dong W-F 2021 Blood pressure assessment with in-ear photoplethysmography *Physiol. Meas.* **42** 105009
- Xing X, Ma Z, Zhang M, Gao X, Li Y, Song M and Dong W-F 2020 Robust blood pressure estimation from finger photoplethysmography using age-dependent linear models *Physiol. Meas.* **41** 025007
- Zhang Z, Pi Z and Liu B 2015 TROIKA: a general framework for heart rate monitoring using wrist-type photoplethysmographic signals during intensive physical exercise *IEEE Trans. Biomed. Eng.* **62** 522–31