



City Research Online

City, University of London Institutional Repository

Citation: Phillips, J. P., Kyriacou, P. A. & Langford, R. M. (2006). Calibration of an optical fibre cerebral oximeter using a Monte Carlo model. Paper presented at the 12th Annual Scientific Meeting of the Institute of Physics and Engineering in Medicine, Sept 2006, Cambridge, UK.

This is the accepted version of the paper.

This version of the publication may differ from the final published version.

Permanent repository link: <https://openaccess.city.ac.uk/id/eprint/14316/>

Link to published version:

Copyright: City Research Online aims to make research outputs of City, University of London available to a wider audience. Copyright and Moral Rights remain with the author(s) and/or copyright holders. URLs from City Research Online may be freely distributed and linked to.

Reuse: Copies of full items can be used for personal research or study, educational, or not-for-profit purposes without prior permission or charge. Provided that the authors, title and full bibliographic details are credited, a hyperlink and/or URL is given for the original metadata page and the content is not changed in any way.

City Research Online:

<http://openaccess.city.ac.uk/>

publications@city.ac.uk

Calibration of an optical fibre cerebral oximeter using a Monte Carlo model.

Phillips J¹, Langford R², Kyriacou P³, Jones D⁴

^{1,2}Anaesthetic Laboratory, St. Bartholomew's Hospital, London, EC1A 7BE

³Department of Engineering and Mathematical Science, City University, London, EC1V 0HB

⁴Medical Electronics and Physics, Department of Engineering, Queen Mary, University of London, E1 0NN

Background and purpose:

In some high-risk patients, such as those recovering from severe head injury, secondary brain damage caused by cerebral ischaemia and/or hypoxia is a common and potentially preventable cause of mortality and residual disability [1]. We are currently developing an optical fibre based system for measuring tissue haemoglobin oxygen saturation with the aim of providing an indicator of cerebral hypoxaemia.

A probe consisting of two parallel optical fibres has been designed for insertion into a trans-cranial bolt allowing the oxygen saturation of blood within the cerebral cortex to be measured. This is achieved by illuminating the tissue with red (660 nm) and infrared (850 nm) light and measuring the backscattered intensity at each wavelength. The optical fibres penetrate approximately 10 mm into the brain tissue and are laterally separated by a distance of 2 mm. A Monte Carlo model was used to develop an algorithm for calculation of oxygen saturation to be calculated from the detected light intensities. The model was validated by comparing results from the model with empirical results obtained from samples of whole blood over a range of oxygen saturation values.

Method:

Blood samples of haematocrit (HCT) = 0.45 with varying oxygen saturation were produced using an IL-237 blood gas tonometer and the oxygen saturation measured on a Radiometer 700 series whole blood oximeter. The red and infrared reflected intensities of these samples were measured with the oximetry system by immersing the probe in each sample and the results compared with results from the model. The absorption coefficient, scatter coefficient and anisotropy factor of blood of varying oxygen saturation were taken from published data. [2]-[3]. The predicted reflected intensities for brain tissue were then calculated using a Monte Carlo model based on published optical coefficients for white matter [4].

Results:

Figure 1 shows a graph of the measured backscattered intensities plotted against oxygen saturation for whole blood, compared with the values

predicted by the Monte Carlo model. It can be seen that there is good correlation between the measured values and the values predicted by the model.

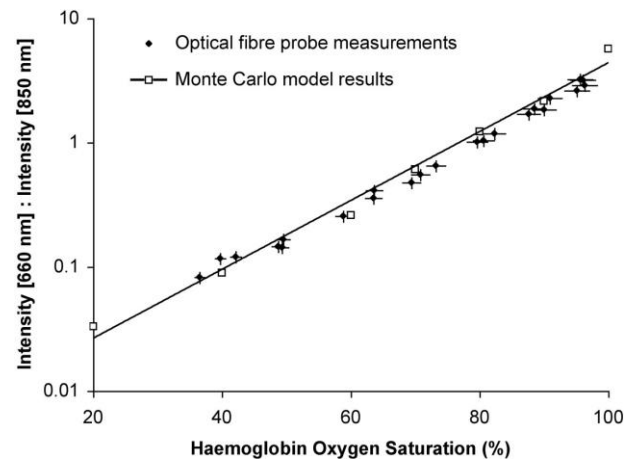


Figure 1: Graph of the ratio of red:infrared backscattered intensity plotted against oxygen saturation for whole blood (HCT = 0.45) as measured by the oximetry probe and as predicted by the Monte Carlo model.

The tissue oxygen saturation ($StiO_2$) for brain tissue, for a cerebral blood volume (CBV) of 0.29%, and an HCT of 0.45 was predicted by the model to be related to the red:infrared intensity ratio (R) by the following linear approximation:

$$StiO_2 = 236.5R - 178.3$$

Conclusions:

The values of the reflected intensities predicted by the model were found to be strongly dependent on the CBV and the HCT. The CBV is known to vary due to autoregulation of cerebral vascular resistance [1]. Using the Monte Carlo model, it would be possible to calculate a series of calibration curves for all values of CBV and HCT in the clinical range. To produce a practical algorithm for the calculation of oxygen saturation would require the CBV to be continuously measured.

References:

- [1] Hinds C, Watson D, Intensive Care - A Concise Textbook, 2nd ed., 1996, Bailliere Tindall, London.
- [2] Wray S, Cope M, Delpy D, Wyatt J, Reynolds E. Characterization of the near infrared absorption spectra of cytochrome aa3 and haemoglobin for the non-invasive monitoring of cerebral oxygenation, Biochim Biophys Acta., 1988: 933: 184-92.
- [3] Roggan A, Friebel M, Dorschel K, Hahn A, Muller G, Optical Properties of circulating human blood in the wavelength range 400-2500 nm, Journal of Biomedical Optics, 1999: 4: 36 - 46.
- [4] Yaroslavsky A, Schulze P, Yaroslavsky I, Schober R, Ulrich F, Schwarzmaier H, Optical properties of selected native and coagulated human brain tissues

in vitro in the visible and near infrared spectral range.
Phys. Med. Biol., 2002: 47: 2059-73.