



## City Research Online

### City, University of London Institutional Repository

---

**Citation:** Vimalakanthan, K., Read, M. G. & Kovacevic, A. (2020). Numerical Modelling and Experimental Validation of Twin-Screw Expander. *Energies*, 13(18), pp. 1-7. doi: 10.3390/en13184700

This is the accepted version of the paper.

This version of the publication may differ from the final published version.

---

**Permanent repository link:** <https://openaccess.city.ac.uk/id/eprint/24875/>

**Link to published version:** <https://doi.org/10.3390/en13184700>

**Copyright:** City Research Online aims to make research outputs of City, University of London available to a wider audience. Copyright and Moral Rights remain with the author(s) and/or copyright holders. URLs from City Research Online may be freely distributed and linked to.

**Reuse:** Copies of full items can be used for personal research or study, educational, or not-for-profit purposes without prior permission or charge. Provided that the authors, title and full bibliographic details are credited, a hyperlink and/or URL is given for the original metadata page and the content is not changed in any way.

---

---



Article

# Numerical Modelling and Experimental Validation of Twin-Screw Expander

Kisorthman Vimalakanthan <sup>1\*</sup>, Matthew Read <sup>1</sup> and Ahmed Kovacevic <sup>1</sup>

<sup>1</sup> City, University of London London, EC1V 0HB, United Kingdom

\* Correspondence: k.vimalakanthan@city.ac.uk (K.V.); m.read@city.ac.uk (M.R.); a.kovacevic@city.ac.uk (A.K.);

Version August 28, 2020 submitted to Energies

**Abstract:** Positive displacement machines have been identified as appropriate expanders for small scale power generation systems such as ORCs. Screw expanders can operate with good efficiency for working fluids under both dry and two-phase conditions. Detailed understanding of the fluid expansion process is required to optimise the machine design and operation for specific applications, and accurate design tools are therefore essential. Using experimental data for air expansion, both CFD and chamber models have been applied to investigate the influence of port flow and leakage on the expansion process. Both models are shown to predict pressure variation and power output with good accuracy. The validated chamber model is then used to identify optimum volume ratio and rotational speed for the experimental conditions.

**Keywords:** twin screw; air; expander; performance; optimisation; chamber model; CFD; validation; built-in volume ratio;

## 1. Introduction

There is currently significant interest in reducing the global greenhouse gas emissions from industrial processes, which alone account for almost 26% (275 Mtoe/yr) of Europe's energy consumption [1]. Studies looking at global thermal energy availability [2] have shown that about 52% of the primary energy consumption is currently being rejected as waste heat. Of this global waste heat potential, 63% exists as low temperature ( $< 100^{\circ}\text{C}$ ) heat sources. Waste heat energy recovery systems seem to be an attractive proposition that can potentially reduce energy consumption and help to decarbonise industrial processes.

The Organic Rankine Cycle (ORC) provides a means of extracting useful electrical or mechanical power from heat sources at low temperature levels. However, this power is extracted with a much lower thermal efficiencies than conventional high temperature Rankine cycles. Additionally, low temperature ORC systems generally demand a larger heat exchange area per unit power generation, resulting in higher investment costs for the heat transfer equipment, with considerable work input for the feed pump due to the lower latent heat of evaporation of the organic fluids compared to water. Conventional ORC cycles are usually limited to dry vapour admission to turbines, which leads to the complication of having to remove the superheat before condensation begins, with an associated increase in the surface area required for heat transfer.


The thermal efficiency of ORCs can generally be increased by allowing a higher mean temperature of heat addition (in accordance with Carnot's principle) or by reducing the mean temperature of heat rejection. By allowing expansion to take place within the two-phase region, the ORC system can achieve a higher mean temperature of heat addition to increase the cycle efficiency, and avoid the requirement to desuperheat the working fluid before the condenser, thereby reducing the mean temperature of heat rejection [3]. Allowing two-phase conditions at the expander inlet also reduces

the constraints due the heat exchanger minimum temperature different, leading to better temperature matching of the heat source and working fluid. This offers the potential to increase heat recovery from the source fluid, thereby increasing the net power output.

The potential thermodynamic and economic benefits of ORC systems, including the Trilateral Flash Cycle [4] and their optimisation [5] considering expansion of initially saturated liquid are reported in the literature. Several studies have also looked at the working fluid selection [6] for working in sub-critical and trans-critical ORC cycles [7] using screw expanders. There is, however, a lack of experimental validation for expander performance models used in these studies.

**Table 1.** Geometrical data of the GL51.2-M twin screw expander

	Male rotor	Female rotor
No of lobes	3	5
Wrap angle	200deg	120deg
Head diameter	72mm	67.5mm
Length		101mm
Built-in volume ratio ( $V_i$ )		1.47
Displaced volume per male rotor revolution		285cm <sup>3</sup>
Rotor profile		mod. asym. SRM-profile
HP/LP ports arrangements		Axial and Radial/Axial
Design Clearance (Interlobe $\times$ Radial $\times$ HP End $\times$ LP End)	50-80 $\mu$ m $\times$ 80 $\mu$ m $\times$ 100 $\mu$ m $\times$ 250 $\mu$ m	

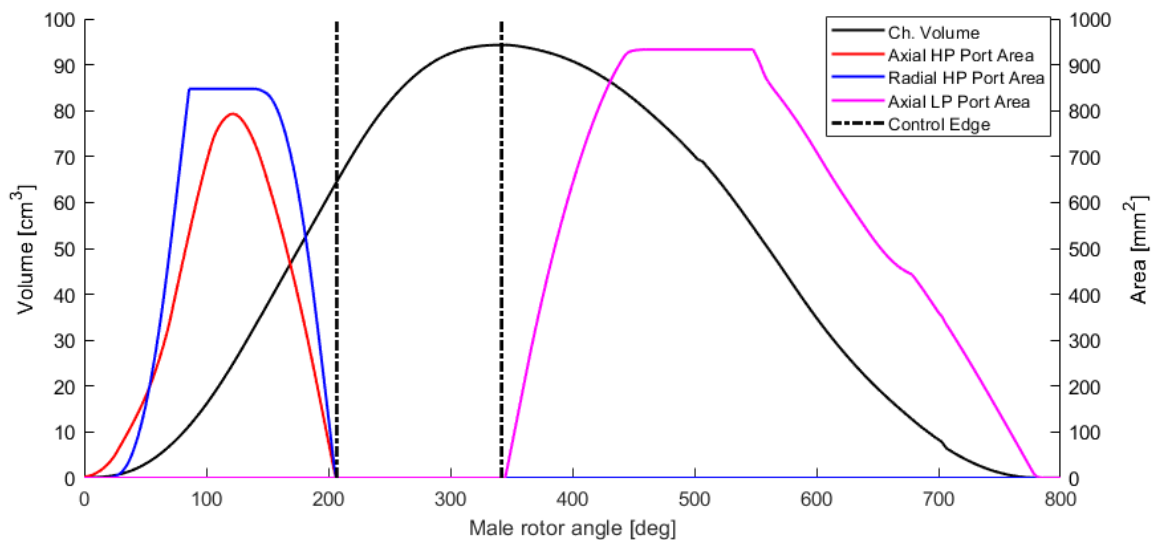

**Figure 1.** Port areas and volume curve of the screw expander GL51.2-M

The expansion of two-phase, liquid vapour mixtures presents serious challenges for turbomachinery, but can be achieved with good efficiency in positive displacement machines. A number of different types of volumetric expander have been considered for use in small-scale ORC systems, as reviewed by Zywnica et al. [8]. The general requirements for high expansion ratio, high isentropic efficiency and low cost mean that scroll, screw, rotary vane and reciprocating piston machines are suitable depending on the necessary working fluid, flow rate and system pressure [9]. For power outputs in the tens of kW, screw expanders have been identified as a suitable expander technology for low temperature waste heat recovery applications. In these applications, expansion of the fluid from saturated liquid [10] or two-phase conditions [3] has been shown to allow maximum net power output from a given waste heat source. However, one of the main challenges with two-phase expansion is the large density change, which influences the physical size requirements for positive displacement machines such as screw expanders.

High efficiency can be achieved by matching the screw expander's built-in volume ratio,  $\epsilon_v$ , to the volumetric expansion of the fluid in the process; the maximum value of  $\epsilon_v$  is however limited due to; geometrical constraints of the screw rotors, increased filling losses due to the decreasing size of the inlet port, and the decreasing mass flow rate for a given machine size. The influence of these different factors makes performance prediction and optimisation of screw expanders essential when considering their use in ORC systems. Thus, it is important to develop a validated model that accurately captures the effect of built-in volume ratio and operating conditions on the expander performance.

This paper will focus on the case of single-phase expansion of air using a twin screw expander. The aim is to establish an accurate and reliable model for the expansion of air, while future work will focus on the more complex case of two-phase expansion, leading to a robust tool for general use in performance prediction of power systems. Two modeling approaches will be considered. Firstly a quasi-1D modelling tool based on the 'chamber model' approach [11] has been developed for twin screw expanders. Secondly, 3D CFD modelling has also been performed for comparison. Previous studies by Kovacevic et al. have described the CFD grid generation and calculation methodology in detail [12] and demonstrated good agreement with measured data for screw expander applications [13]. The numerical results were computed for the expander with characteristics defined in (Table 1 and Figure 1) running on single-phase air and compared against the experimental data presented by Hutker et. al. [14]. An extension of this work validating two-phase R245fa expansion is the focus of future research publications. For single or two-phase conditions, the validated model allows evaluation of maximum efficiency maps as a function of built-in volume ratios at different pressure ratios. This will be demonstrated for the air expander considered in this paper. These established performance maps can be used with cycle optimisation tools to evaluate the optimum design of twin-screw expander geometry and its operating conditions for specific applications within power generation systems.


## 2. Modelling

Two numerical modelling approaches for twin-screw expanders are presented in this section. The first is a 1D chamber model (1D Ch. Model), which is a computationally efficient approach to solve the system of equations. The second approach considers the expander in its three-dimensional (3D CFD) numerical environment and models the full three-dimensional Navier-Stokes equations with RANS k-e closure for turbulence modelling, which requires several days of computation on high performance clusters. The in-house computational code SCORG© [13] enables use of both chamber modelling and 3D CFD in screw machines.

### 2.1. Chamber model (1D Ch. Model)

Based on the geometry calculation from SCORG V5.7 (Figure 1), the commercial software GT-SUITE [15] was used to implement the multi chamber modelling approach outlined in the [11]. This software models working chamber of the expander and manifolds using chamber modelling, where scalar variables are assumed to be uniform within, while all other flow component are modelled using 1D formulation of the Navier-Stokes equations on a staggered grid spatial discretisation.

The expander is divided into various fluid components (Figure 2) such that an inlet pipe connecting a flow-split that feeds the working chambers of the expander, which then allows the fluid to accumulate to another flow split and exit via outlet pipe work. The pipe volumes are divided into sub volumes while the chamber and flow split manifolds are represented by a single volume, while the vector variables are solved at the boundary.

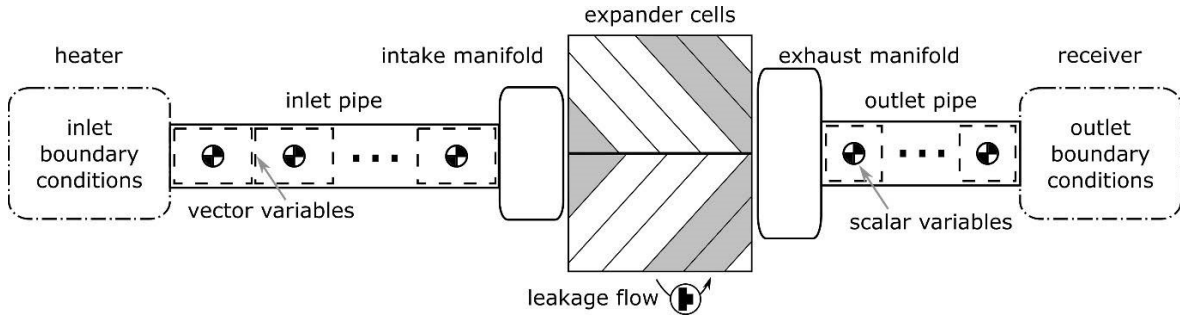

**Figure 2.** Modelling approach for 1D Ch. Model [10]


The chamber volume and the corresponding flow areas for ports and leakage paths are provided as a function of rotor angle (Figure 1). Currently, no heat transfer is modelled and the walls of the components are modelled as adiabatic.

All fluid components within the 1D Ch. Model including leakage flows are modelled as flow through an orifice. For the validation case considering gaseous air, the orifice flow is modelled based on the isentropic nozzle relationships for subsonic and choked flow regimes.

For the two-phase environment, the nozzle flow is modeled using incompressible Bernoulli equation for liquids, and the isentropic nozzle relationships are considered for gases. This requires the calculation of ratio of specify heat ( $\gamma$ ) and dynamic viscosity ( $\mu$ ), which are calculated as an equivalent property using a weighted average based on the fluid quality ( $\chi$ ) as shown in Eq. (1) and Eq. (2).

$$\gamma_{eqv} = \gamma_{vap}\chi + \gamma_{liq}(1 - \chi) \quad (1)$$

$$1/\mu_{eqv} = \chi/\mu_{vap} + (1 - \chi)/\mu_{liq} \quad (2)$$

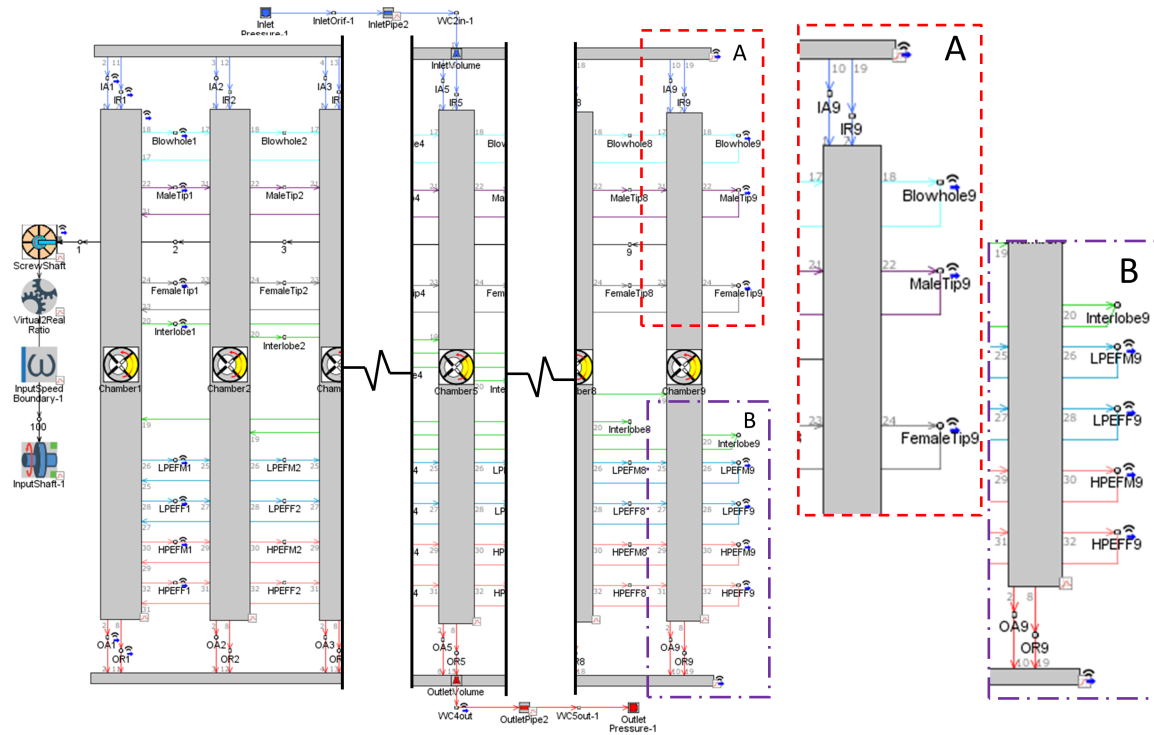

**Figure 3.** GT-SUITE model of GL51-M Expander, IA = inlet axial port, IR= inlet radial port, OA = outlet axial port, OR = outlet radial port, Male Tip = male rotor tip clearance leakage, Female Tip = female rotor tip clearance leakage, LPEFM = low pressure end face male rotor leakage, LPEFF = low pressure end face female rotor leakage, HPEFM = high pressure end face male rotor leakage, HPEFF = high pressure end face female rotor leakage,


The systems of conservation equations are solved using explicit 5th order Runge-Kutta integration scheme to solve for mass and internal energy. With the known volume and mass, the corresponding density is calculated. The density and internal energy values are used to then determine the pressure and temperature via the NIST REFPROP database [16].

The GT-SUITE model implementation of the twin-screw GL51.2-M expander is shown in Figure 3. The 3/5 lobed machine is modelled with 9 chambers in total, which is calculated based on the maximum number of working chambers that the meshing rotors can form at a point in time. All chambers are connected to the inlet and outlet manifolds and dedicated links are modelled for axial and radial ports respectively. The leakage paths are also modelled via their own dedicated connections between the chambers, and it is connected via a cyclic link where the last chamber is connected to the first chamber in order to allow continuity and leakage access to all possible paths.

The explicit solver was set to consider a maximum time step corresponding to  $1^\circ$  solving the equation for the full cycle ( $360^\circ$ ). The convergence criteria set at steady-state condition on mass flow rate and pressure, i.e. 0.2% variation on mass flow rate and pressure in flow connections compared with the results from the previous cycle.

## 2.2. Computational Fluid Dynamics Model (3D CFD)


To assess the quality of the 1D Ch. Model discussed in the previous section, 3D CFD simulations were conducted and compared against the experimental data. As the working fluid flows through the machine, the net force exerted by the fluid on the rotors causes rotation, with expansion of the fluid occurring once the inlet port closes (Figure 4). This results in net power output via the shaft of the male rotor, which can be used to drive a mechanical load or electrical generator.

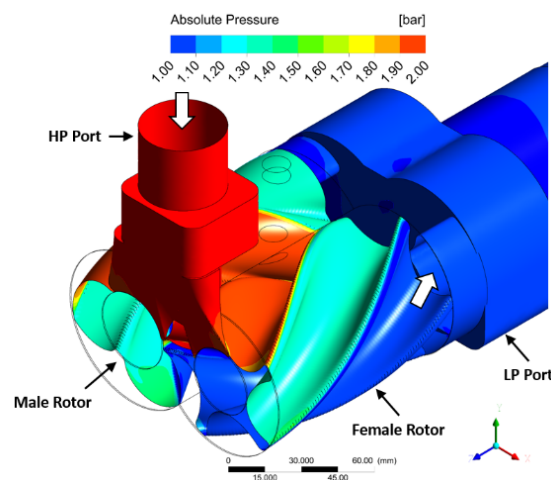

**Figure 4.** Pressure variation in twin screw expander

The computational fluid domain is decomposed into three main regions (Figure 5) namely the high pressure (HP) port, rotor domain (containing the male and female rotor) and the low pressure (LP) port. Moreover, the end face clearances were modelled with additional domains attached on both sides of the rotor; i.e. the HP end face leakage was modelled with additional domain discretising the space between the HP port and rotor. A numerical (GGI) interface was used to connect all the computational domains. The rotor domain is updated with a corresponding grid at each time intervals to model the rotation.



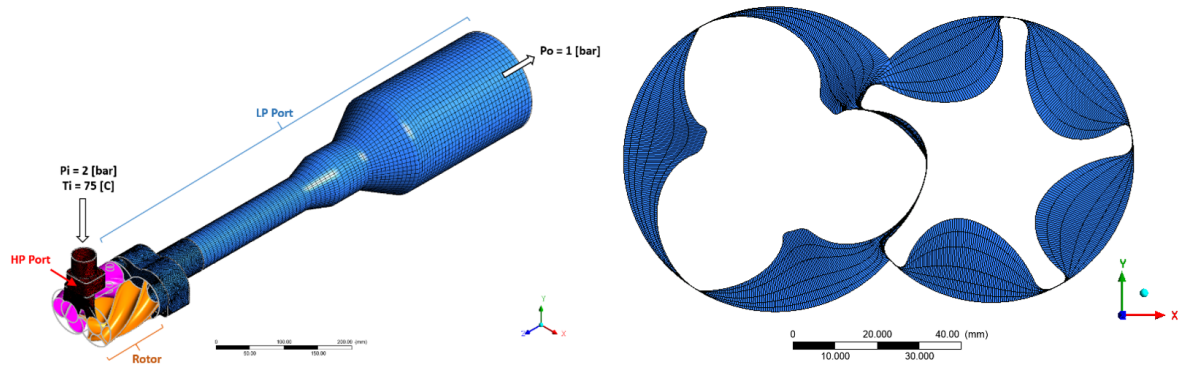

**Figure 5.** CFD domains with surface mesh for the GL51.2-M twin screw expander

The convergence criteria for mass, momentum and energy equations were set to an r.m.s value of  $1\text{E-}4$ ,  $1\text{E-}3$  and  $1\text{E-}3$  respectively. Surplus amount of time steps were considered for all simulations until a cyclic repetition were observed for pressure, power and mass flow rate via the machine.

### 3. Results

Numerical simulations were conducted to replicate the experimental conditions reported in [14]. A range of inlet pressures between 1.5-3bar was investigated at an inlet temperature of  $75\text{C}$ , with the expander rotational speed ranging from 1,000-16,000RPM.

The design clearance gaps for the GL51-2M expander were defined as  $50\text{-}80\mu\text{m}$  for the interlobe,  $80\mu\text{m}$  radial and 100 and  $250\mu\text{m}$  for the high-pressure (HP) and low-pressure (LP) end faces respectively. However, due to mechanical and thermal loads these clearance gaps are known to change in operation. Operational clearance settings of  $10\times 80\times 640\times 10\mu\text{m}$  corresponding to the interlobe, radial, HP end face and LP end face were chosen for both numerical simulations. This clearance setting was evaluated based on a genetic optimisation routine that minimises the differences between the computed and measured power and mass flow values, while closely matching the measured internal pressure curve at 2bar inlet pressure with 4,000RPM rotational speed.

#### 3.1. Validation Results


The results from both 3D CFD and 1D chamber models agree well with the measured indicated power (Figure 6 and Table 2) at the lower rotational speeds.

**Table 2.** Indicated power and mass flow rates for 4,000 and 10,000RPM

	n = 4,000RPM		n = 10,000RPM	
	Power [kW]	Mass flow [kg/s]	Power [kW]	Mass flow [kg/s]
Exp	1.464	0.0450	3.445	0.0790
1D Ch. Model	1.477	0.0456	3.552	0.0809
3D CFD Model	1.442	0.0536	3.239	0.0834

The predicted power values from the chamber model are within 2% of the measurements ( $<8,000\text{RPM}$ ). However, the overall results (Figure 6) clearly show that the accuracy of the numerical simulations deteriorates with increasing rotational speeds, specifically beyond 10,000RPM.



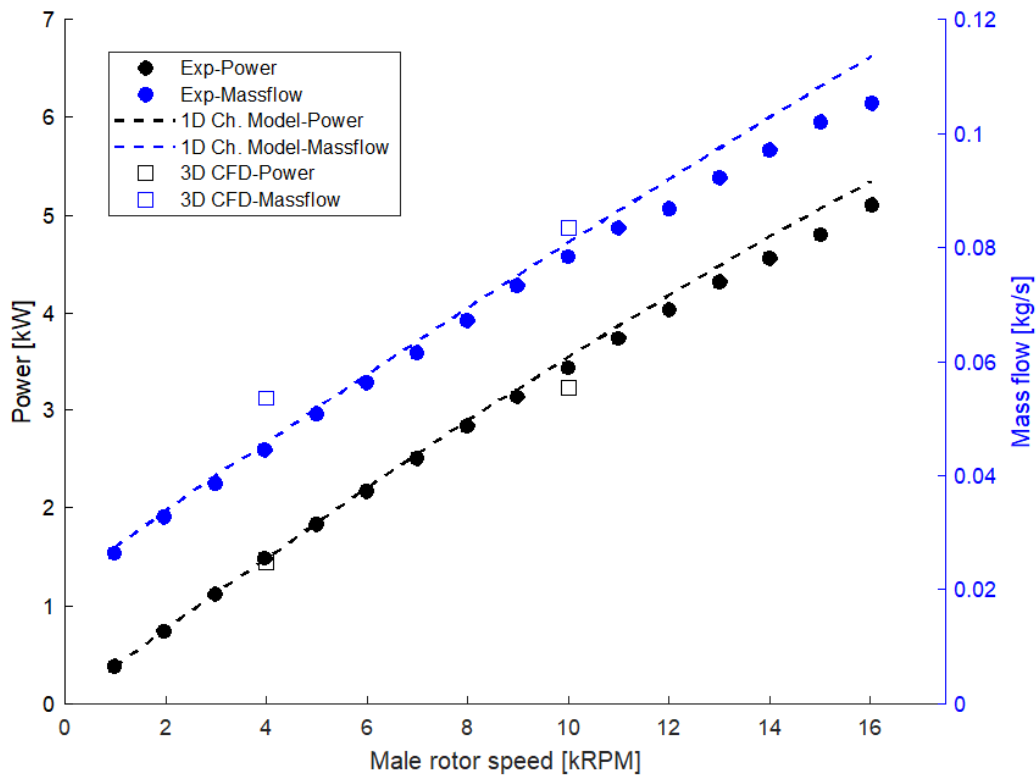


**Figure 6.** Measured and calculated indicated power and mass flow as a function of rotational speed [ $P_i = 2\text{bar}$ ,  $T_i = 75^\circ\text{C}$ ]

The 3D CFD model consistently under-predicts the power output and over-predicts the mass flow rates for both simulated rotational speeds, while the chamber model predicts slightly larger power output and mass flowrates. Details validation study comparing the internal pressure traces are presented in Figure 7 and 8 for the two rotational speeds shown in Table 2), which is discussed in the following section.


At the 4,000RPM, the CFD model significantly over-predicts the mass flow rates by 19% and under-predicts the power output by 1.5%, which results in a substantial under-prediction of the expander's specific power output (17%). The specific power output of an expander is a measure of its isentropic and mechanical efficiency and the chamber model accurately compute the specific power within 1% of the measurements. At the larger rotational speed of 10,000RPM the CFD results show better prediction of the mass flow rate and the difference with measurement is reduces to 6%.

The validation study is conducted using the internal pressure measurements for different rotational speeds: 4,000 (Figure 7) and 10,000RPM (Figure 8), for the inlet pressure of 2bar. The results show that both numerical models compute the indicated pressures with reasonable accuracy. The filling (up to 208 deg) and refilling (caused by net leakage of fluid into the working chamber between 250-380 deg) trends seen from the measurements are captured well with both numerical models.

Negligible differences are found between the chamber and high-fidelity 3D CFD models at the 4,000RPM. At the higher rotational speed of 10,000RPM, the low fidelity chamber model utilizing simple orifice equations shows better prediction for the filling losses than the CFD results, at the 2bar inlet pressure.

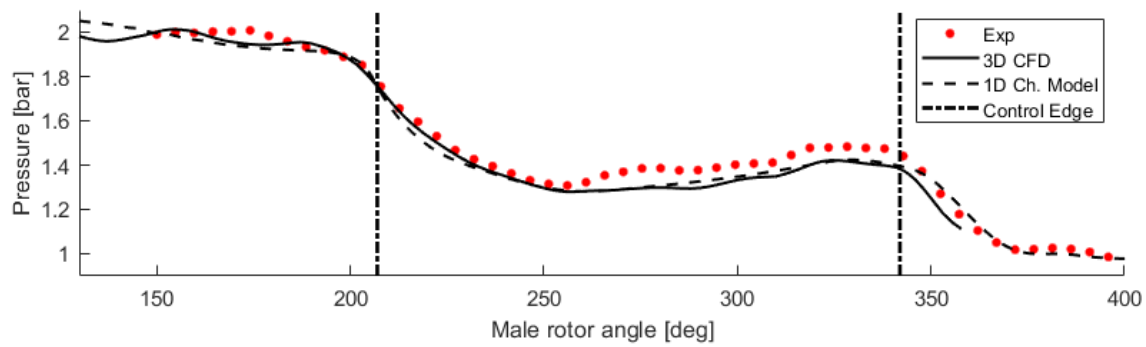


**Figure 7.** Validation of simulated pressure curves against male rotor's rotational angle [ $n=4,000\text{RPM}$ ,  $P_i=2\text{bar}$ ,  $T_i=75\text{C}$ ]

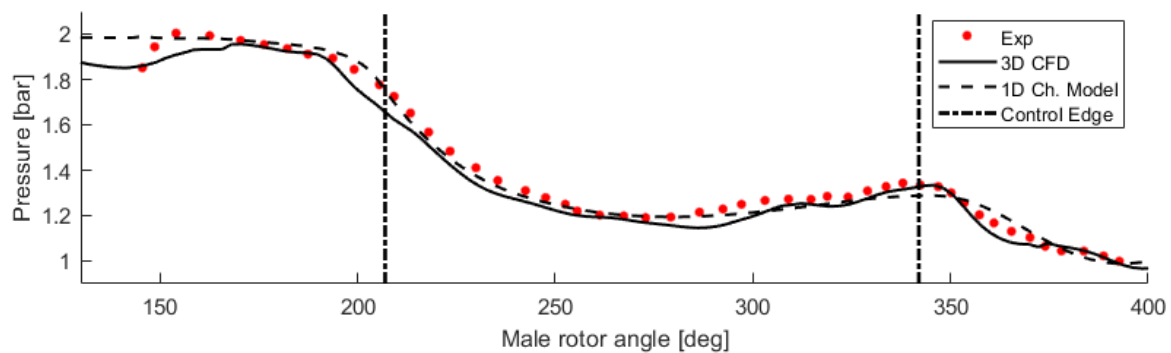


**Figure 8.** Validation of simulated pressure curves against male rotor's rotational angle [ $n=10,000\text{RPM}$ ,  $P_i=2\text{bar}$ ,  $T_i=75\text{C}$ ]

Comparing the indicated diagrams for different inlet pressures at the rotational speed of 10,000RPM (Figure 10) reveals that the chamber model consistently underpredicts the filling losses with increasing inlet pressures (or density). A 6% difference in filling pressure is found between the chamber model predictions and measurement, at the highest inlet pressure of 3bar. However, the results also show that refilling losses are accurately predicted with the chamber model. This suggests that despite modelling the leakages with reasonable accuracy, the orifice assumption based on isentropic nozzle relationship is insufficient to accurately capture the losses incurred via the high-pressure port, especially at the large pressure ratios (3:1).

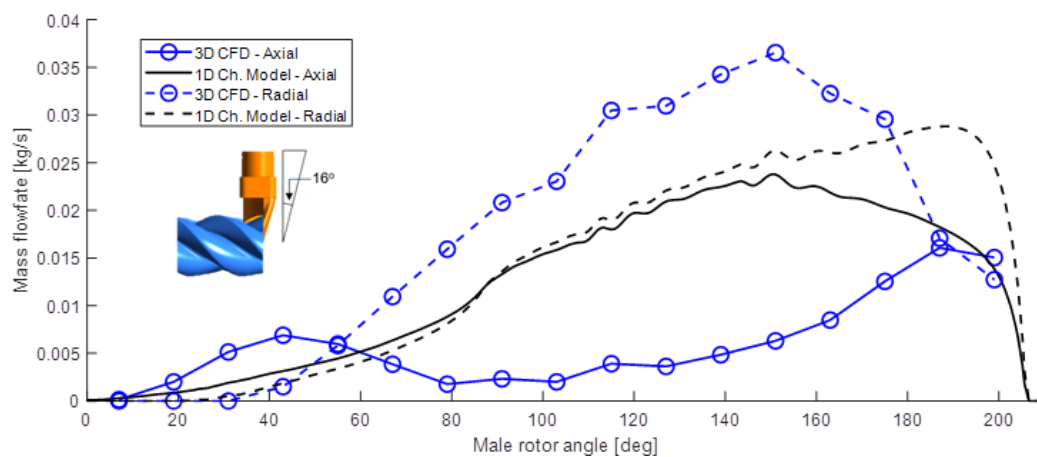

**Figure 9.** High pressure flow characteristics for the GL51.2-M twin screw expander [ $P_i=2\text{bar}$ ,  $n=4,000\text{RPM}$ ]

Based on the post processed results, it was clear that the two numerical models calculate significantly different flow characteristics to each other (Figure 9). The CFD model simulating the actual three-dimensional port geometry (16deg flow angle) calculates much larger flow via the radial port than the axial, while the chamber model with orifice assumption (90deg) shows similar proportion of the flow via both ports until 150deg of the male rotor position, where flow through the radial port dominates.

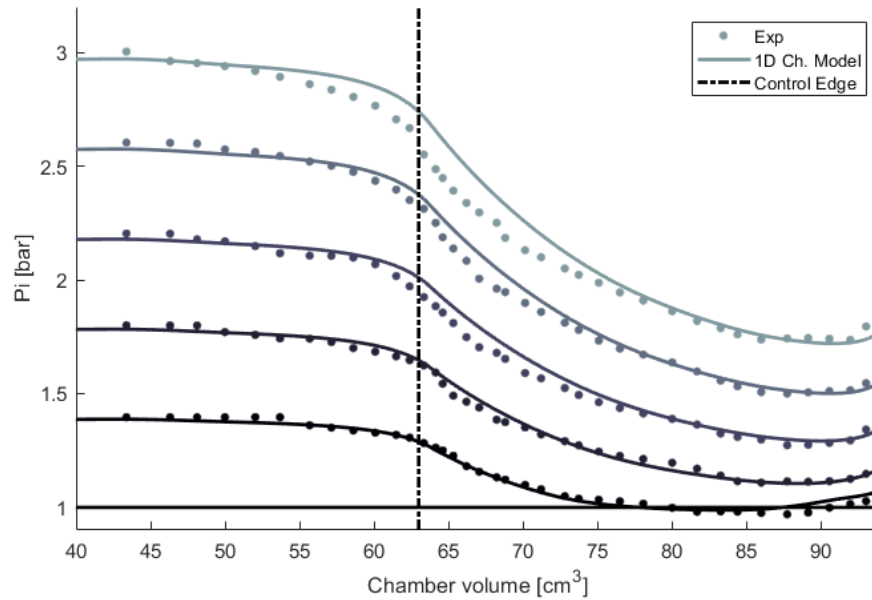

**Figure 10.** Validation of simulated indicated diagrams for different inlet pressure [ $n=10,000\text{RPM}$ ,  $T_i=75\text{C}$ ]

These results stress the need for an improved model for the high-pressure port. One possibility is to account for a restricted flow via the axial port based on the skewed geometry, such as using reduced port area profile based on the components of the flow directions. Improving the flow characteristics based on the 3D port geometry likely to achieve higher accuracy using the chamber model approach.


### 3.2. Maximum efficiency maps

The isentropic efficiency of a twin-screw expanders depends on the built-in volume ratio ( $\epsilon_v$ ) the actual volumetric expansion ratio of the fluid and the rotational speed. The built-in volume ratio is a function of the high-pressure port geometry, while the volumetric expansion ratio is based on the inlet and outlet fluid conditions. These two parameters determine the expanders' ability to match the expansion occurring within the machine to the required application. At higher rotational speeds the leakage become a lower proportion of the mass flow rate, resulting in higher maximum isentropic efficiency when operating with a suitable value of  $\epsilon_v$ . Increasing rotational speed tends to increase the pressure drop during filling of the working chambers; this pre-expansion of the fluid can lead to optimum values of  $\epsilon_v$  well below the volumetric expansion ratio for the process. Accurate modelling is therefore necessary when assessing system performance and optimum expander design.


Using the established Chamber model, the maximum isentropic efficiency map was evaluated using the steps below for this expander running on air:

1. Inlet pressure,  $P_i$ , is fixed
2.  $\dot{m}$  and  $\eta$  calculated for the range of  $\omega$  and  $\epsilon_v$  values
3. Maximum values of  $\eta$  (and corresponding values of  $\omega$  and  $\epsilon_v$ ) identified as a function of  $\dot{m}$
4. Repeat steps 1-3 across the range of  $P_i$  values
5. Calculated data allows contour plots of maximum  $\eta$  and corresponding  $\epsilon_v$  and  $\omega$  values as functions of  $P_i$  and  $\dot{m}$


214 The range of values considered for the input parameters was;  $1 \leq \epsilon_v \leq 10$  in steps of 0.5,  $500 \leq \omega \leq$   
 215 16,000 RPM in steps of 500 RPM, and  $1.5 \leq P_i \leq 3$  bar in steps of 0.25 bar. A constant outlet pressure  
 216 of 1 bar was used in all cases. The resulting contour maps are shown in Figures 11–13.

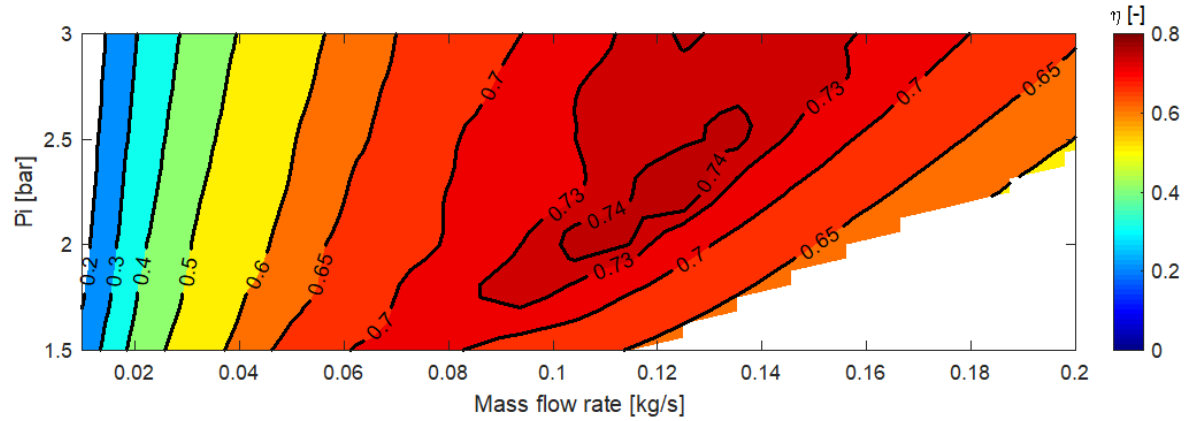

**Figure 11.** Maximum efficiency map for GL51 twin-screw expander running on air [Ti=75C, Po=1bar]

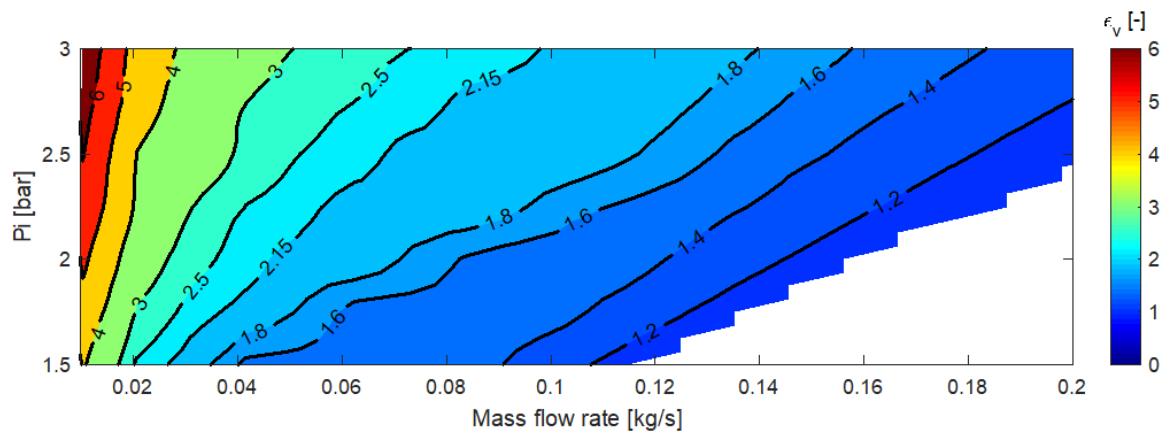

**Figure 12.** Built-in volume ratio ( $\epsilon_v$ ) corresponding to maximum isentropic efficiency of GL51 twin-screw expander running on air [Ti=75C, Po=1bar]

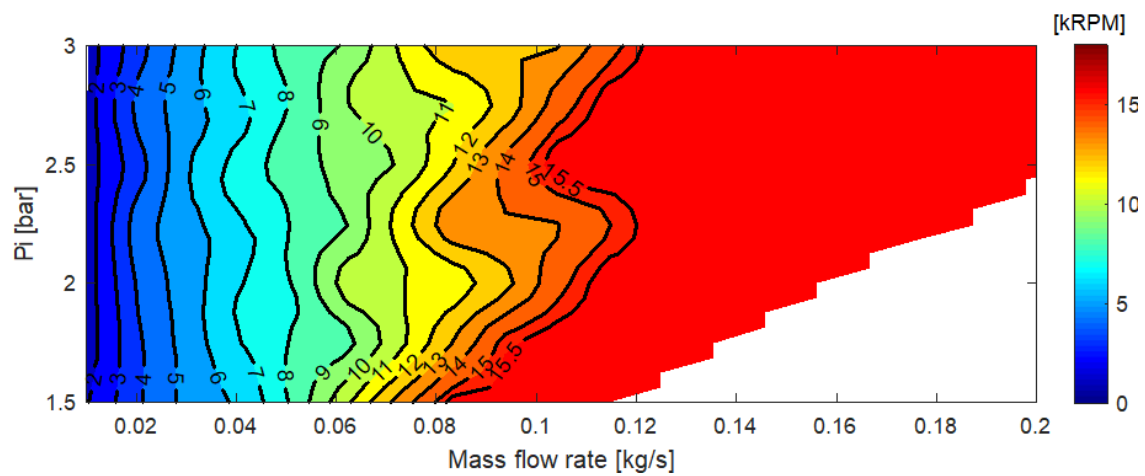

**Figure 13.** Rotational speeds corresponding to maximum isentropic efficiency of GL51 twin-screw expander running on air [Ti=75C, Po=1bar]

Based on the results (Figure 11), the better efficiency operation is achieved with increasing mass flow rates up to 0.07kg/s for all investigated inlet pressures. The global optimum efficiency is achieved at mass flow rates between 0.100-0.140kg/s with inlet pressures of 2.1-2.6bar respectively. This range of operation with maximum efficiency is achieved with a close to constant volume ratio of  $\epsilon_v = 1.6$  (Figure 12) for rotational speeds above 15,500RPM (Figure 13). Larger mass flow rates beyond 0.14kg/s, shows reduction in maximum efficiency. The losses during filling meaning that the pressure at the start of expansion is relatively low, which effectively reduces the work done (area of the pV diagram), resulting in less mass per cycle and less work per cycle. The pressure drop across the inlet port means that there is lost work, and so specific work tends to decrease at higher speeds.

For the conditions above the 15,000RPM, the experimented machine configuration with  $\epsilon_v$  of 1.47 was found to be operating close to the best conditions suggested by the maximum efficiency maps. At the experimented condition with inlet pressure of 2bar and mass flow rate of 0.102kg/s, the experimentally established isentropic efficiency was found to be 0.7, while the optimum operation recommended by the efficiency map (Figure 11) for 2bar inlet pressure with 0.102kg/s is with  $\epsilon_v=1.49$  where the machine achieves an isentropic efficiency of 0.74.

#### 4. Conclusions

Positive displacement machines have been identified as appropriate expanders for small scale power generation systems such as ORCs. Detailed understanding of the fluid expansion process is required to optimise the machine design and operation for specific applications, and accurate design tools are therefore essential.

Using experimental data for air expansion, both CFD and chamber models have been applied to investigate the numerical accuracy on the power output and mass flowrate. A detailed validation study was conducted using the measured internal pressure curves to assess the leakage and the filling loss predictions. Both models are shown to predict pressure variation and power output with good accuracy. However, results also indicates that the accuracy of the numerical predictions deteriorates with increasing rotational speeds and increasing inlet densities. These finding suggests that further investigations are required to quantify and assess the simple orifice assumption considered for leakage and filling loss predictions. Nevertheless, the validated chamber model has been successfully used to demonstrate the process of determining the optimum built-in volume ratio and rotational speed for the experimented conditions.

An extension of this work validating two-phase R245fa expansion is published at the Rankine2020 conference [17].

**Author Contributions:** Conceptualization, K.V., M.R. and A.K.; methodology, K.V. and M.R.; validation, K.V.; formal analysis, K.V.; investigation, K.V.; resources, A.K.; data curation, K.V.; writing—original draft preparation, K.V.; writing—review and editing, K.V., M.R. and A.K.; visualization, K.V.; supervision, M.R. and A.K.; All authors have read and agreed to the published version of the manuscript.

**Funding:** This research was funded by EPSRC (Grant number: EP/P009131/1).

**Acknowledgments:** Authors would like to thank Prof Andreas Brummer and Technical University of Dortmund for providing geometry and experimental results of GL-51 expander

**Conflicts of Interest:** The authors declare no conflict of interest.

#### Abbreviations

The following abbreviations are used in this manuscript:

Exp	Experimental
1D Ch. Model	One dimensional chamber model
3D CFD Model	Three dimensional computational fluid dynamics model

## References

1. Panayiotou, G.P.; Bianchi, G.; Georgiou, G.; Aresti, L.; Argyrou, M.; Agathokleous, R.; Tsamos, K.M.; Tassou, S.A.; Florides, G.; Kalogirou, S.; others. Preliminary assessment of waste heat potential in major European industries. *Energy Procedia* **2017**, *123*, 335–345.
2. Forman, C.; Muritala, I.K.; Pardemann, R.; Meyer, B. Estimating the global waste heat potential. *Renewable and Sustainable Energy Reviews* **2016**, *57*, 1568–1579.
3. Read, M.; Smith, I.; Stosic, N.; Kovacevic, A. Comparison of organic Rankine cycle systems under varying conditions using turbine and twin-screw expanders. *Energies* **2016**, *9*, 614.
4. Fischer, J. Comparison of trilateral cycles and organic Rankine cycles. *Energy* **2011**, *36*, 6208–6219.
5. Read, M.; Smith, I.; Stosic, N. Optimisation of power generation cycles using saturated liquid expansion to maximise heat recovery. *Proceedings of the Institution of Mechanical Engineers, Part E: Journal of Process Mechanical Engineering* **2017**, *23*, 57–69.
6. Kolasinski, P. The Method of the Working Fluid Selection for Organic Rankine Cycle (ORC) Systems Employing Volumetric Expanders. *Energies* **2020**, *13*, 573.
7. Zhang, X.; Zhang, Y.; Cao, M.; Wang, J.; Wu, Y.; Ma, C. Working fluid selection for organic Rankine cycle using single-screw expander. *Energies* **2019**, *12*, 3197.
8. Zywicka, G.; Kaczmarczyk, T.Z.; Ihnatowicz, E. A review of expanders for power generation in small-scale organic Rankine cycle systems: Performance and operational aspects. *Proceedings of the institution of mechanical engineers, part A: journal of power and energy* **2016**, *230*, 669–684.
9. Bao, J.; Zhao, L. A review of working fluid and expander selections for organic Rankine cycle. *Renewable and Sustainable Energy Reviews* **2013**, *24*, 325 – 342. doi:<https://doi.org/10.1016/j.rser.2013.03.040>.
10. Bianchi, G.; Kennedy, S.; Zaher, O.; Tassou, S.A.; Miller, J.; Jouhara, H. Numerical modeling of a two-phase twin-screw expander for Trilateral Flash Cycle applications. *International Journal of Refrigeration* **2018**, *88*, 248–259.
11. Stosic, N.; Smith, I.K.; Kovacevic, A. Calculation of Screw Compressor Performance. *Screw Compressors: Mathematical Modelling and Performance Calculation* **2005**, pp. 49–75.
12. Kovacevic, A.; Rane, S. Algebraic generation of single domain computational grid for twin screw machines Part II–Validation. *Advances in Engineering Software* **2017**, *109*, 31–43.
13. Rane, S.; Kovačević, A.; Stošić, N. Grid Generation for CFD Analysis and Design of a Variety of Twin Screw Machines. *Designs* **2019**, *3*, 30.
14. Hütker, J.; Brümmer, A. Physics of a dry running unsynchronized twin screw expander. *Proceedings of the 8th International Conference on Compressors and their Systems*, London, UK, 2013, pp. 9–10.
15. Manual, G.P.U. GT-Suite™ Version 2019. *Gamma Technologies* **2019**.
16. Lemmon, E.; Huber, M.; McLinden, M. NIST Standard Reference Database 23, Reference Fluid Thermodynamic and Transport Properties (REFPROP), version 9.0, National Institute of Standards and Technology. *R1234yf. fld file dated December* **2010**, *22*, 2010.
17. Vimalakanthan, K.; Read, M.; Kovacevic, A. Performance Prediction and Optimisation of Twin-Screw Expander. *IIR International Rankine 2020 Conference - Heating, Cooling and Power Generation; International Institute of Refrigeration*, 2020. DOI: 10.18462/iir.rankine.2020.146.

**Sample Availability:** Samples of the compounds ..... are available from the authors.

© 2020 by the authors. Submitted to *Energies* for possible open access publication under the terms and conditions of the Creative Commons Attribution (CC BY) license (<http://creativecommons.org/licenses/by/4.0/>).